



TIRF microscopy as a screening method for non-specific binding on surfaces

Christy Charlton^{a,*}, Vladimir Gubala^a, Ram Prasad Gandhiraman^a, Julie Wiechecki^a, Nam Cao Hoai Le^a, Conor Coyle^{a,b}, Stephen Daniels^{a,b}, Brian D. MacCraith^a, David E. Williams^{a,c}

^a Biomedical Diagnostics Institute, Dublin City University, Dublin 9, Ireland

^b National Center for Plasma Science and Technology, Dublin City University, Dublin 9, Ireland

^c MacDiarmid Institute for Advanced Materials and Nanotechnology, Department of Chemistry, University of Auckland, Private Bag 92019, Auckland 1142, New Zealand

ARTICLE INFO

Article history:

Received 1 September 2010

Accepted 13 October 2010

Available online 20 October 2010

Keywords:

Total internal reflection

Fluorescence

Microscopy

Non-specific binding

Surface-particle interaction

ABSTRACT

We report a method for studying nanoparticle-biosensor surface interactions based on total internal reflection fluorescence (TIRF) microscopy. We demonstrate that this simple technique allows for high throughput screening of non-specific adsorption (NSA) of nanoparticles on surfaces of different chemical composition. Binding events between fluorescent nanoparticles and functionalized Zeonor[®] surfaces are observed in real-time, giving a measure of the attractive or repulsive properties of the surface and the kinetics of the interaction. Three types of coatings have been studied: one containing a polymerized aminosilane network with terminal $-NH_2$ groups, a second film with a high density of $-COOH$ surface groups and the third with sterically restraining branched poly(ethylene)glycol (PEG) functionality. TIRF microscopy revealed that the NSA of nanoparticles with negative surface charge on such modified coatings decreased in the following order $-NH_2 > \text{branched PEG} > -COOH$. The surface specificity of the technique also allows discrimination of the degree of NSA of the same surface at different pH.

© 2010 Elsevier Inc. All rights reserved.

1. Introduction

Current research in biomedical diagnostics is directed at inexpensive, highly sensitive, miniaturized devices, in which usually disposable substrates or chips are used. Such devices are required to measure analytes in microliter volume samples, typically at picomolar level. In fluorescence-based assays, the signal can be greatly enhanced with the use of dye-doped nanoparticles as fluorescent labels [1–4]. However, in a successful diagnostics device, signal-to-noise ratio is paramount to its performance and effectively controls the sensitivity. Controlling the noise and background contribution, dictated by non-specific binding of the non-analyte constituents of the sample remains very challenging. The chemical composition of the substrate surface and its interactions with the active surface area of the dye-doped nanoparticles, therefore, play a key role in the performance of diagnostic platform. In this work, we focus on surface functionalization of the substrate Zeonor[®], a cyclo-olefin polymer (COP), which is characterized by ease of injection molding for biochip fabrication and relatively low auto-fluorescence, which is an important factor for fluorescence-based applications including TIRF microscopy.

Total internal reflection fluorescence (TIRF) microscopy [5] is presented here as a very useful and fast method to compare

non-specific adsorption of detection molecules on different surfaces. This method allowed for rapid screening of surfaces to find their ability to prevent non-specific binding. Total internal reflection occurs at any interface between materials of different refractive index inside the material of higher refractive index provided the angle of incidence of the light is above the critical angle defined as:

$$\theta_c = \arcsin \left(\frac{n_2}{n_1} \right) \quad (1)$$

where n_1 is the refractive index of the high refractive index material (Zeonor[®] ≈ 1.5 in our case but this could also be glass or other polymers) and n_2 is the refractive index of the low index material (typically water = 1.3 or air = 1). Upon total internal reflection, an evanescent field is established which penetrates a small distance (in our case, approx. 100 nm) into the low refractive index material. TIRF is typically achieved by coupling excitation light to the surface through either a prism or the microscope objective [5]. More recently, excitation light has been coupled into a waveguide and microscopic measurements have been performed on the waveguide surface [6]. In our experiments, light is coupled directly into a $2.5 \times 7 \times 0.2$ cm slide fabricated from cyclo-olefin polymer, known commercially as Zeonor[®], to allow for characterization of surface coatings by simply counting the adsorbed particles on the substrate. TIRF allows surface-particle interactions to be investigated, as it excites only particles within the evanescent field of the excitation light, providing surface specificity and improving signal to noise compared with conventional microscopy [5]. In this work, we use TIRF in a novel way to

* Corresponding author. Address: Biomedical Diagnostics Institute, Dublin City University, National Center for Sensor Research, Research and Engineering Building, Glasnevin, Dublin 9, Ireland. Fax: +353 1 700 6558.

E-mail address: christy.charlton@dcu.ie (C. Charlton).

screen surfaces for the levels of non-specific binding in a particular system.

We have recently reported that fluorescent nanoparticles are very useful as labels in immunoassays to achieve improvements both in assay kinetics and sensitivity [7–9]. However, these particles typically have a negatively charged surface due to surfactants used to stabilize them and avoid aggregation [10,11]. This can cause particles to bind non-specifically due to charge attraction to surfaces commonly used for protein absorption such as 3-aminopropyltriethoxy silane (APTES) [12–14]. As illustrated on Scheme 1, APTES coated substrates contain a high density of amine groups that are in equilibrium between the charged —NH_3^+ and neutral —NH_2 form. Whether this equilibrium is shifted towards its charged or neutral species depends on the pH of the environment. At physiological pH, it is the effect of the positively charged —NH_3^+ groups that governs the surface characteristics. It is therefore expected that the physical adsorption of negatively charged nanoparticles on such a surface would be high due to a favourable electrostatic attraction with the —NH_3^+ groups. On the other hand, a film that is intrinsically negatively charged, such as one with —COOH functional groups, is expected to significantly reduce the non-specific adsorption of the nanoparticles. Indeed, the carboxy group is mostly deprotonated (shown as —COO^- in Scheme 1) at $\text{pH} \sim 7$. Such coating was prepared by co-polymerization of acrylic acid and tetraorthosilicate (TEOS) using a method called plasma enhanced chemical vapour deposition (PECVD). In this process, TEOS was grafted onto a Zeonor substrate and allowed to cross-link with molecules of acrylic acid. The polymerization reaction was initiated by plasma and resulted in the formation of exceptionally stable, hydrophilic film with high density of —COOH groups.

Polyethylene(glycol) derivatives are also known in surface chemistry as effective suppressors of non-specific binding of biomolecules [15–18]. Their function is associated less with electrostatic forces but rather with vast hydration and effects of change of configurational entropy when large molecules adsorb upon them. We have modified an APTES film with a branched and sterically demanding PEG derivative (Scheme 1) and compared the physisorption of nanoparticles with both charged coatings. Surface particle density and binding rate constants were used as a measure of surface–particle attraction; the effect of the pH was also investigated. We show that kinetic data can be extracted from the real-time binding curves of the particles on each surface. This tool could be used to investigate surface binding kinetics, which are another key parameter in diagnostic devices [19,20].

2. Materials and methods

2.1. Fluorescent particles

Carboxyl functionalized yellow fluorescent polystyrene nanoparticles (110 nm diameter, 1.0% w/v solution in water, FITC

compatible dye with excitation max at 470 nm and emission max at 490 nm) were purchased from Kisker Biotech (Steinfurt, Germany). The stock solution was diluted to a final concentration of 1×10^{-4} mg/mL in deionized water for the surface comparison measurement and in 0.1 M 2-(N-morpholino)ethanesulfonic acid (MES) buffer at pH values of 3 and 7 for the pH comparison measurements. Buffers were made using 0.1 M MES and adjusted with HCl to pH 3 and with NaOH to pH 7.

2.2. NP – anti-hCG conjugation


One milligram of fluorescent amine functionalized (170 nm diameter) fluorescent polystyrene NPs was washed two times in water by centrifugation (17,000 rpm, 10 min), then resuspended in 0.5 mL of 0.1 M NaHCO_3 buffer at $\text{pH} = 8.5$. To this mixture, 117 μg of monoclonal anti β -hCG antibody was added and allowed to physically adsorb on the surface of the polystyrene NPs in the course of 3 h. The unreacted, free anti β -hCG in solution was removed by centrifugation and the mixture was washed three times with phosphate buffered saline at $\text{pH} = 7.4$. For longer term storage, bovine serum albumine (BSA) would be added to the sample and it would be kept in a dark, cold place.

2.3. Surface preparation

Microscope size slides ($2.5 \times 7.0 \times 0.2$ cm) were made of Zeonor® and supplied by Åmic and Sigolis (Uppsala, Sweden). One set of slides were coated with a 93 Å thick layer of polymerized molecules of 3-aminopropyltriethoxy silane (APTES) and ethylenediamine (EDA) by plasma enhanced chemical vapour deposition (PECVD) [21]. PEG functionalized slides were prepared by immersing the APTES coated slides in a 1 mM solution of TMS(PEG)_{12} with 2.5 + 5.2 nm long spacer arm, purchased from Pierce Chemicals. COOH functionalized Zeonor® slides were prepared using PECVD [22] technique by co-polymerization of tetraorthosilicate and acrylic acid. A cartoon of surfaces coatings are shown in Scheme 1. Our PECVD coated surfaces have been shown to have a roughness of approx. 1 nm [12,13]. This roughness is minimal and does not effect the surface measurements presented in this work.

2.4. TIRF setup

A 473 nm blue laser with 50 mW maximum output (Photop Technologies Inc, Fujian, China) was coupled to the Zeonor® microscopy slide via a BK7 prism (BRP-5, Newport, Oxfordshire, UK) index matched to the slide with immersion oil. Light entered the slide at an angle of 15° from horizontal giving an angle of reflection at the Zeonor®/water interface of approximately 65° from the vertical, which is above the critical angle of 61° needed for total internal reflection. This setup was placed above the

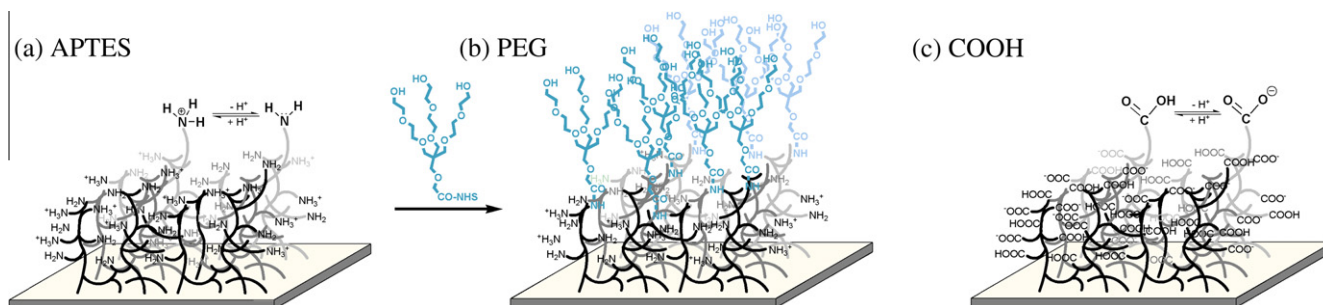

Scheme 1. Schematic of surface functionalizations: (a) APTES, (b) PEG and (c) Carboxyl.

objective on an Olympus IX81 (Olympus, Essex, UK) inverted fluorescence microscope. A drop of fluorescent particle solution was placed on the top slide surface at a location where the laser beam was being reflected from the surface giving an evanescent field at that point. When the particles reach the surface, they are excited by the evanescent field and emit fluorescence which is collected through the slide from below. The TIRF setup is shown schematically in Fig. 1a and pictorially in Fig. 1b.

2.5. Imaging and particle counting

A 20×0.50 NA objective (UPlanFLN, Olympus, Essex, UK) was used giving a viewing area of 0.144 mm^2 . An Olympus U-MWIBA filter was used to block excitation light of the laser and image the fluorescence emitted by the particles. Images were recorded every 10 s for 2000 s with a 5 s exposure time on an Olympus DP71 camera. Image color was adjusted using ImageJ software to remove background noise before particles were counted using Matlab image processing software.

3. Results and discussion

The fluorescent nanoparticles used in our experiments have carboxyl functional groups that are mostly negatively charged in water or buffered solutions at $\text{pH} \sim 7$ for improved colloidal stability (zeta potential was measured to be -36 mV for particles in $\text{pH} 7$ MES buffer). Three types of coatings were studied. Two sets with deposited molecules that can be either positively (protonated $-\text{NH}_2$ groups) or negatively (deprotonated $-\text{COOH}$ groups) charged under the measured conditions. A third coating had neutral PEG grafted on top of the APTES film forming an additional layer of 7.7 nm thick. While the branched PEG linker does not possess any charge, it is an example of highly hydrated surface as it has the ability to interact with large number of water molecules. Pristine COP is a relatively hydrophobic material with a water contact angle $>90^\circ$. Treatment of COP with the chemicals to obtain coatings as described above rendered the surface more hydrophilic with water contact angles decreasing in the order $-\text{NH}_2 > \text{PEG} > -\text{COOH}$ (Table 1).

Fig. 2 shows three selected images illustrating the accumulation of NPs on the studied surfaces over time. Note that the recorded image of a particle is a convolution of the geometric particle image of diameter M_{dp} , with the diameter of the diffraction-limited point spread function (PSF) of the recording optics, $d_{s\infty}$. The diameter of

Table 1

Water contact angle values of the prepared coatings, the average particle density for each surface calculated at a time of 2000 s and the corresponding binding rate constants.

Surface	Water contact angle (degrees)	Average surface NP density (particles/ mm^2)	Binding rate constant $k_{2000} \text{ (s}^{-1}\text{)}^b$
APTES	55.0 ± 2.6	5727 ± 185	$83 \times 10^{-2} \pm 1.9$
TMS(PEG) ₁₂	38.3 ± 1.5	1537 ± 387	$25 \times 10^{-2} \pm 1.1$
COOH at $\text{pH} 7$	9.9 ± 0.2	206 ± 16	$2 \times 10^{-2} \pm 0.3$
COOH at $\text{pH} 3$		951 ± 84	$8 \times 10^{-2} \pm 0.2$
COOH at $\text{pH} 7^a$		387 ± 53	$6 \times 10^{-2} \pm 0.4$

^a The nanoparticles in this experiment were sensitized with monoclonal anti-hCG antibody and the values were analyzed at a time of 1000 s.

^b The binding rate constants were calculated by fitting a linear regression to the first 250 s of each measurement curve shown in Fig. 3.

the diffraction-limited PSF of an infinity-corrected system can be calculated as [23]:

$$d_{s\infty} = 1.22M\lambda \left[\left(\frac{n_0}{NA} \right)^2 - 1 \right]^{1/2} \quad (2)$$

where n_0 is the refractive index of the immersion medium (air, $n_0 = 1$), $NA = 0.5$ and $M = 20$ are the numerical aperture and magnification of the objective lens, respectively, $d_p = 110 \text{ nm}$ is the particle nominal diameter and $\lambda = 490 \text{ nm}$ is the wavelength of emission maxima of the fluorescent particle. For the system reported here, the diffraction-limited PSF size is calculated to be $20.7 \mu\text{m}$.

The particle image diameter can be obtained by approximating M_{dp} and $d_{s\infty}$ as Gaussians [24]:

$$d_e = [M^2 d_p^2 + d_{s\infty}^2]^{1/2} \quad (3)$$

The particle image diameter is calculated to be $20.8 \mu\text{m}$, which projected back to the surface of the substrates, would correspond to $1.04 \mu\text{m}$. This explains the apparent size of the particles in Fig. 2.

Image processing algorithms allowed a particle count to be determined for each image giving the number of particles on the surface at each individual time frame. The results were then plotted as a function of NP count vs. time for APTES, PEG, and COOH surfaces as shown in Fig. 3a.

As expected, the negatively charged NPs were mostly attracted to the amine terminated APTES surface groups. The average density of surface bound NPs at a time of 2000 s was nearly 28 times higher than that of the negatively charged $-\text{COOH}$ surface. If the

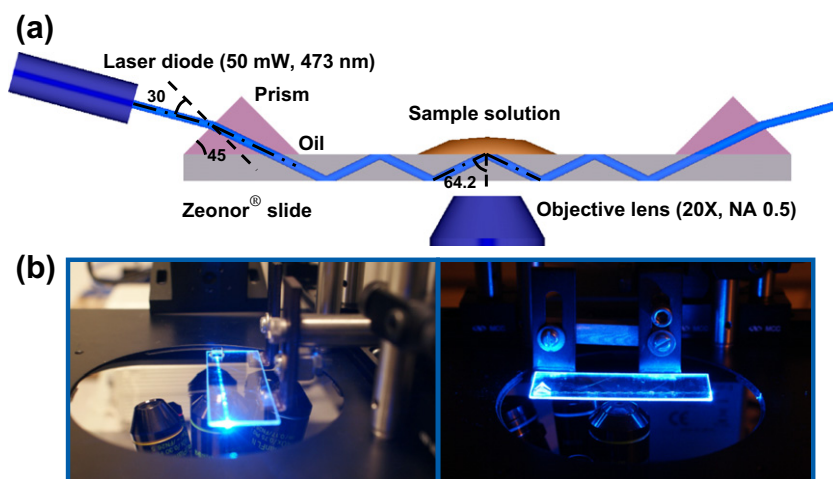


Fig. 1. (a) Schematic of TIRF setup; (b) photos of TIRF setup.

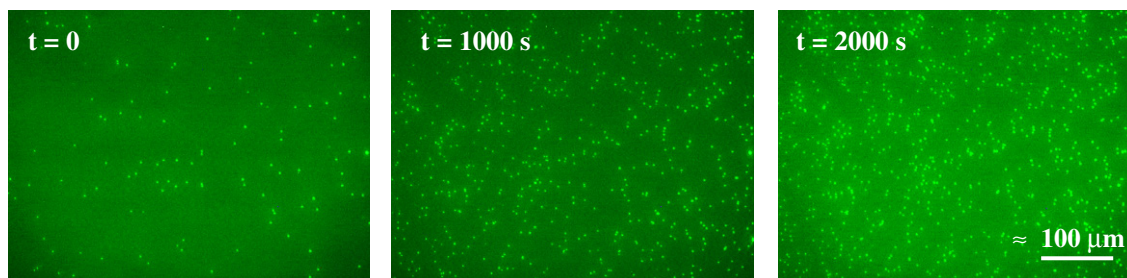


Fig. 2. Images of particle accumulation on surface for an APTES coated slide (note: color brightened to enhance particle visibility). (For interpretation of the references to color in this figure legend, the reader is referred to the web version of this article.)

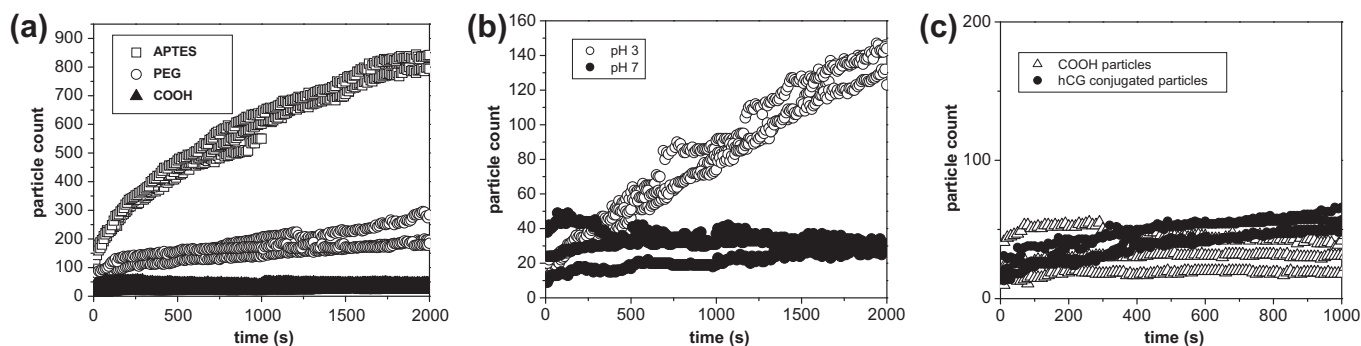


Fig. 3. Graph of particle count vs. time for carboxylated particles accumulating on each of the following surfaces: (a) APTES ($\square$), PEG ($\circ$) and COOH ($\blacktriangle$); (b) COOH at pH 3 ($\circ$) COOH at and pH 7 ($\bullet$); (c) COOH surface with COOH functionalized particles ($\triangle$) COOH surface with hCG conjugated particles ($\bullet$).

particle coverage on the surface is sufficiently low that the particle accumulation on the surface is not affected by particle–particle interactions or by the approach to the jamming limit, then the accumulation can be described as a simple first-order chemical reaction. The rate constant can be obtained by fitting and determination of the initial rate of rise. Rate constants were determined based on an average of the three curves for each surface shown in Fig. 3. The difference between the relative binding rate constant of the two charged surfaces was more than 40-fold (Table 1). In comparison with the APTES film, the neutral PEG modified slides showed only a 4-fold decrease in the number of adsorbed NPs and 3-fold decrease in the binding rate constant (k_{2000})_{rel}. Despite the positive effect of the PEG layer acting as a steric, highly hydrated barrier, we reason that it is the electrostatic interactions that dominate the physical adsorption of the negatively charged nanoparticles on the substrate surface.

With that in mind, we further investigated the effect of varying solution pH on the NP accumulation. Since the pKa value for the –COOH groups is in the range of 4.2–5.0, at pH values below this, the equilibrium between –COOH and –COO[−] will be shifted to the protonated form, hence reducing the charge effect of the film. As a consequence, more NPs were expected to accumulate on such surface. This phenomenon was demonstrated in buffered solution at pH = 3 and summarized on Fig. 3b. By neutralizing the charge both on the surface of the particles and on the substrate, the average surface density of the bound NPs along with its binding rates increased by a factor of 4.

For the negatively charged, neutral or near-neutral surfaces, the imaging revealed that the surface was in small, isolated patches not compositionally uniform. We deduce this from the fact that some particles adhered very rapidly (within the time taken to focus the microscope – ~ 10 s) after which the accumulation rate decreased significantly. This effect was particularly noticeable for the nominally neutral PEG-modified surface (Fig. 3a) and for the carboxylate-coated surface at pH7 (Fig. 3b).

In fluorescence-based immunoassays, the dye-doped nanoparticles are sensitized with the detection antibody, which obviously has an impact on the overall charge of the label. Therefore, we reviewed the effect of non-specific binding of antibody-sensitized NPs on the carboxyl functionalized surface. Monoclonal anti β -hCG antibody was immobilized on the surface of the fluorescent NPs and their accumulation on the –COOH surface (so far confirmed to be the most effective in reducing non-specific binding) was monitored in course of 1000 s. The results are summarized on Fig. 3c, comparing the effect of unmodified NPs with the antibody-sensitized NPs. As the isoelectric point of anti-hCG antibody is below the pH of the solution (7), it is assumed that its overall charge is negative. Consequently, the antibody immobilized on the NP surface did not drastically change the total negative charge of the particle. The net result is only a small increase in non-specific binding when compared to that of unmodified NPs, what is ultimately a very important parameter for improving signal-to-noise ratio in any diagnostics device.

4. Conclusion

We have shown that TIRF microscopy can be used as a simple rapid screening tool for non-specific interactions between fluorescent particles and surfaces. This method can be used to determine what surface characteristics are the most optimal for a given application, resulting in the lowest levels of non-specific binding. From our studied surfaces, it is the like-charge electrostatic repulsion between substrate and NPs that showed the strongest effect in decreasing the background signal. The charge–charge repulsions greatly outperformed the effect of PEG coatings that function on the basis of steric hindrance and water hydration. COOH functionalized surfaces were found to provide enough charge repulsion even to the antibody coated particles, leading to very low non-specific binding. The TIRF technique is clearly extremely useful for the study of the surface related interactions in a full immunoassay.

Acknowledgment

The authors wish to thank Martin Sommers for assistance with image processing. We are grateful to Science Foundation Ireland (Grant No. 05/CE3/B754) for funding.

References

- [1] A. Burns, H. Ow, U. Wiesner, *Chem. Soc. Rev.* 35 (2006) 1028.
- [2] C.E. Fowler, B. Lebeau, S. Mann, *Chem. Commun.* (1998) 1825.
- [3] V. Gubala, X. Le Guevel, R. Nooney, D.E. Williams, B.D. MacCraith, *Talanta* 81 (2010) 1833.
- [4] J.L. Yan, M.C. Estevez, J.E. Smith, K.M. Wang, X.X. He, L. Wang, W.H. Tan, *Nano Today* 2 (2007) 44.
- [5] H. Schneckenburger, *Curr. Opin. Biotechnol.* 16 (2005) 13.
- [6] A. Hassanazadeh, M. Nitsche, S. Mittler, S. Armstrong, J. Dixon, U. Langbein, *Appl. Phys. Lett.* 92 (2008) 233503.
- [7] C. Crean (née Lynam), V. Gubala, R. O'Kennedy, D.E. Williams, *Mater. Chem. Phys.* submitted for publication.
- [8] V. Gubala, C. Lynam, R. Nooney, S. Hearty, B. McDonnell, R. O'Kennedy, D.E. Williams, *Anal. Bioanal. Chem.*, submitted for publication.
- [9] C. McDonagh, O. Stranik, R. Nooney, B.D. MacCraith, *Nanomedicine* 4 (6) (2009) 645.
- [10] R.J. Hunter, *Foundations of Colloid Science*, vol. 1, Oxford University Press, New York, 1987.
- [11] R.I. Nooney, C.M.N. McCahey, O. Stranik, X. Le Guevel, C. McDonagh, B.D. MacCraith, *Anal. Bioanal. Chem.* 393 (4) (2009) 1143.
- [12] R.P. Gandhiraman, C. Volcke, V. Gubala, C. Doyle, J. Raj, L. Basabe-Desmonts, M. Iacono, R.I. Nooney, G. Herzog, S. Daniels, D.W.M. Arrigan, B. James, D.E. Williams, *J. Mater. Chem.* 20 (2010) 4116.
- [13] V. Gubala, R.P. Gandhiraman, C. Volcke, C. Doyle, C. Coyle, B. James, S. Daniels, D.E. Williams, *Analyst* 135 (2010) 1375.
- [14] C. Jonsson, M. Aronsson, G. Rundstrom, C. Pettersson, I. Mendel-Hartvig, J. Bakker, E. Martinsson, B. Liedberg, B. MacCraith, O. Ohman, J. Melin, *Lab Chip* 8 (2008) 1191.
- [15] P.K. Ajikumar, J.K. Ng, Y.C. Tang, J.Y. Lee, G. Stephanopoulos, H.-P. Too, *Langmuir* 23 (2007) 5670.
- [16] T. McPherson, A. Kidane, I. Szleifer, K. Park, *Langmuir* 14 (1998) 176.
- [17] S. Pasche, J. Voros, H.J. Griesser, N.D. Spencer, M. Textor, *J. Phys. Chem. B* 109 (37) (2005) 17545.
- [18] A.J. Pertsin, M. Grunze, *Langmuir* 16 (2000) 8829.
- [19] K.E. Sapsford, Z. Liron, Y.S. Shubin, F.S. Ligler, *Anal. Chem.* 73 (22) (2001) 5518.
- [20] K.E. Sapsford, F.S. Ligler, *Biosens. Bioelectronics* 19 (2004) 1045.
- [21] G. Ram Prasad, S. Daniels, D.C. Cameron, B.P. McNamara, E. Tully, R. O'Kennedy, *Surf. Coat. Technol.* 200 (2004) 1031.
- [22] C. Coyle et al., Patent and manuscript in preparation.
- [23] C.D. Meinhardt, S.T. Wereley, *Meas. Sci. Technol.* 14 (2003) 1047.
- [24] R.J. Adrian, *Annu. Rev. Fluid Mech.* 23 (1991) 261.